



# Dog Ovulation Detector

data sheet

Name

	date	hour	result
1			
2			
3			
4			
5			
6			
7			
8			
9			
10			
11			
12			
13			
14			
15			
16			
17			
18			
19			
20			

	date	hour	result
21			
22			
23			
24			
25			
26			
27			
28			
29			
30			
31			
32			
33			
34			
35			
36			
37			
38			
39			
40			

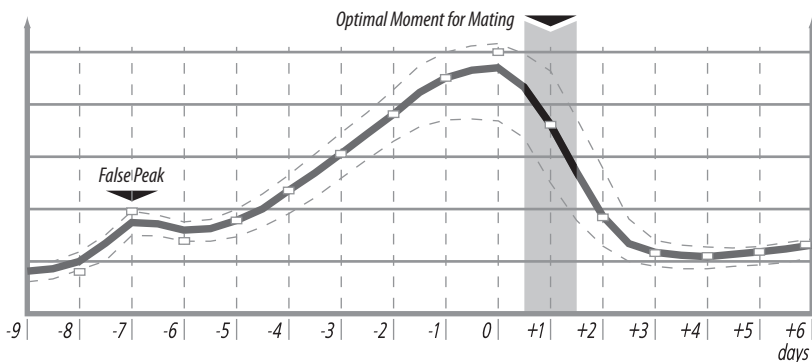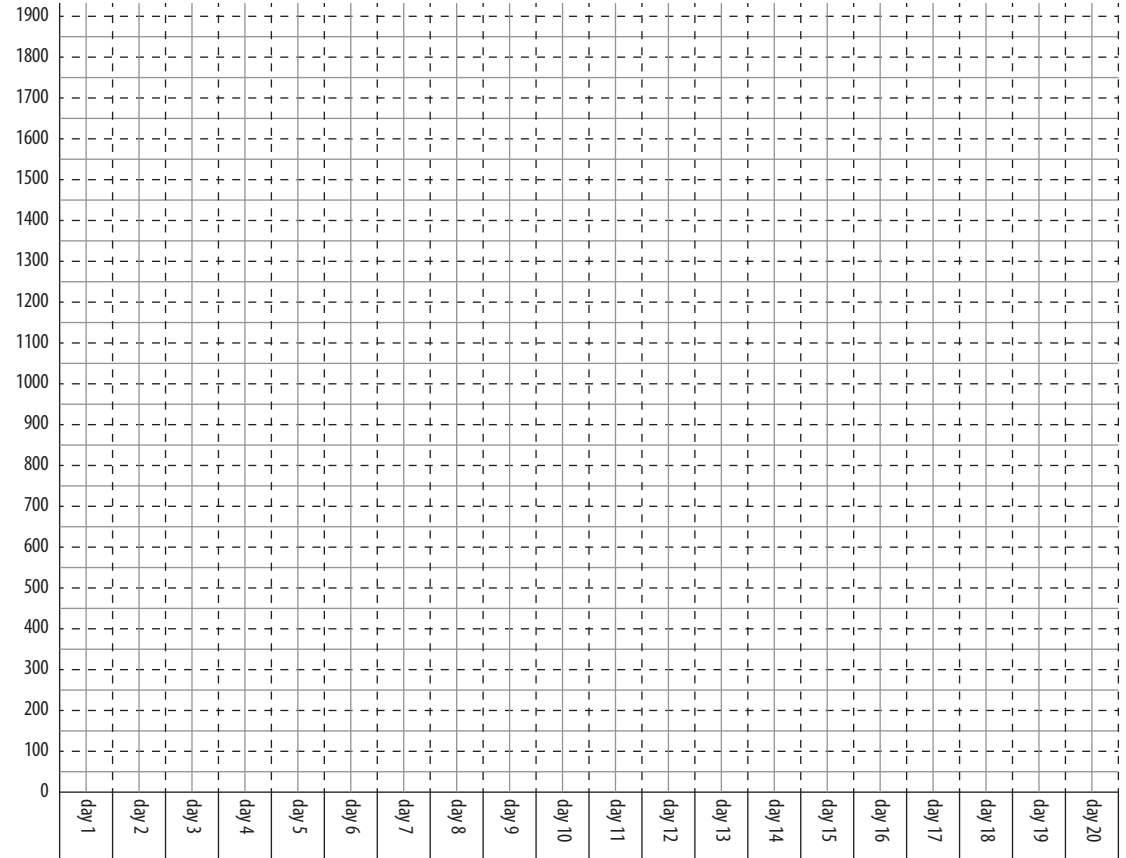

Example of a graph

**Remember to:**

- disinfect the probe
- remove the residual urine or other dirt from the vulva
- perform measurements always at the same depth
- rotate the probe inside the vagina before pressing the button
- perform measurements on a regular basis (2–4 times per day)

**Always remember about the hygiene and disinfection of the probe before and after each use**